

Vootto Air Purifier LTD

February 2nd

Raising the bar in air purifier technology.

2021



Report No:ATCCR20082102F

Antiviral test

ISO-18184 Test Protocol

Sample Category	Media without coating (Heat treatment)
Client	AL(SHANGHAI)AUTOMOTIVE CO.,LTD
Test Category	Test Entrust
Date of Report	2020.09.08

北京京畿分析测试中心有限公司
Analytical and Testing Center of Capital Regions

Vootto Air Purifier LTD


February 2nd

Raising the bar in air purifier technology.

2021

Detection Information

Client	AL(SHANGHAI)AUTOMOTIVE CO.,LTD		Sample Source	Inspect
Client address	NO.3575 Feng Zhe Rd.Feng Xian,Shanghai		Sample State	Normal
Date of Receives samples	2020.08.10		Date(s) of tests	2020.08.10-2020.09.08
Sample No	ATCCR20082102F-0821CP01			
Category	Test Project	Test Standard and Method		Test Instruments
Media without coating (Heat treatment)	Antiviral Activity Value (SARS-CoV-2)	ISO 18184:2019 Textiles Determination of antiviral		Biosafety Cabinet
End				
Remarks	Color: Brown			
Report Preparer:	刘畅		Authorized Signatory:	
Report Reviewer:	李强		Issue Date of Report: 2020.09.08 (Special Chapter for Inspection and Inspection)	

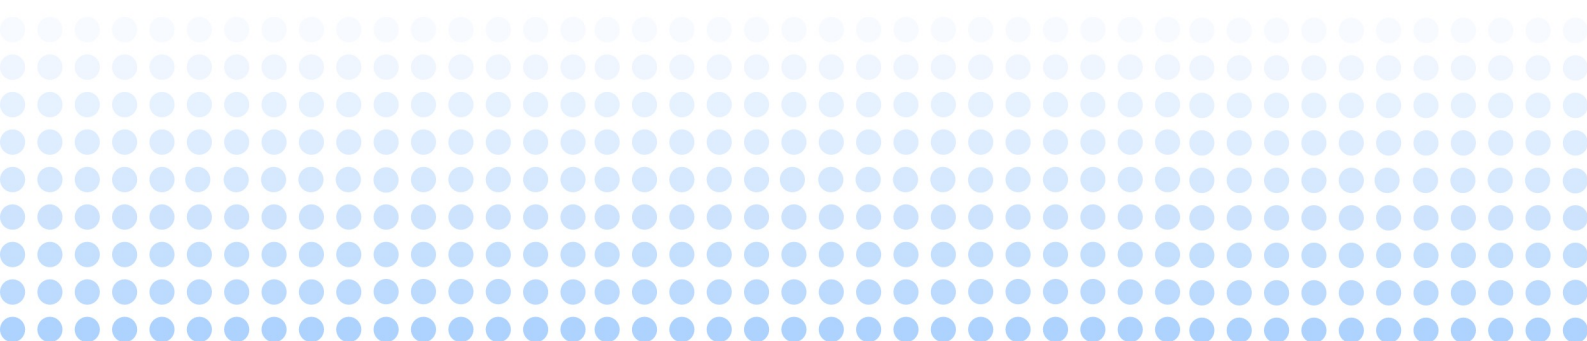


Vootto Air Purifier LTD

February 2nd

Raising the bar in air purifier technology.

2021

Test Results

Virus Types	NO	lg(Va _{0t}) (lgTCID ₅₀ /mL)	lg(Vb _{2t}) (lgTCID ₅₀ /mL)	lg(Vc _{2t}) (lgTCID ₅₀ /mL)
SARS-CoV-2 Virus MDCK	1	6.67	6.42	4.4
	2	6.65	6.48	4.5
	3	6.69	6.53	4.3
Average Value of lgTCID ₅₀ /mL		6.67	6.48	4.41
Antiviral Activity Value		2.07		
Antiviral Activity Rate (%)		99.15		
 <p>End</p> 